




CJC 1295 with DAC peptide compounded 2mg vial

High Pressure Liquid Chromatography test completed on 19/07/2023

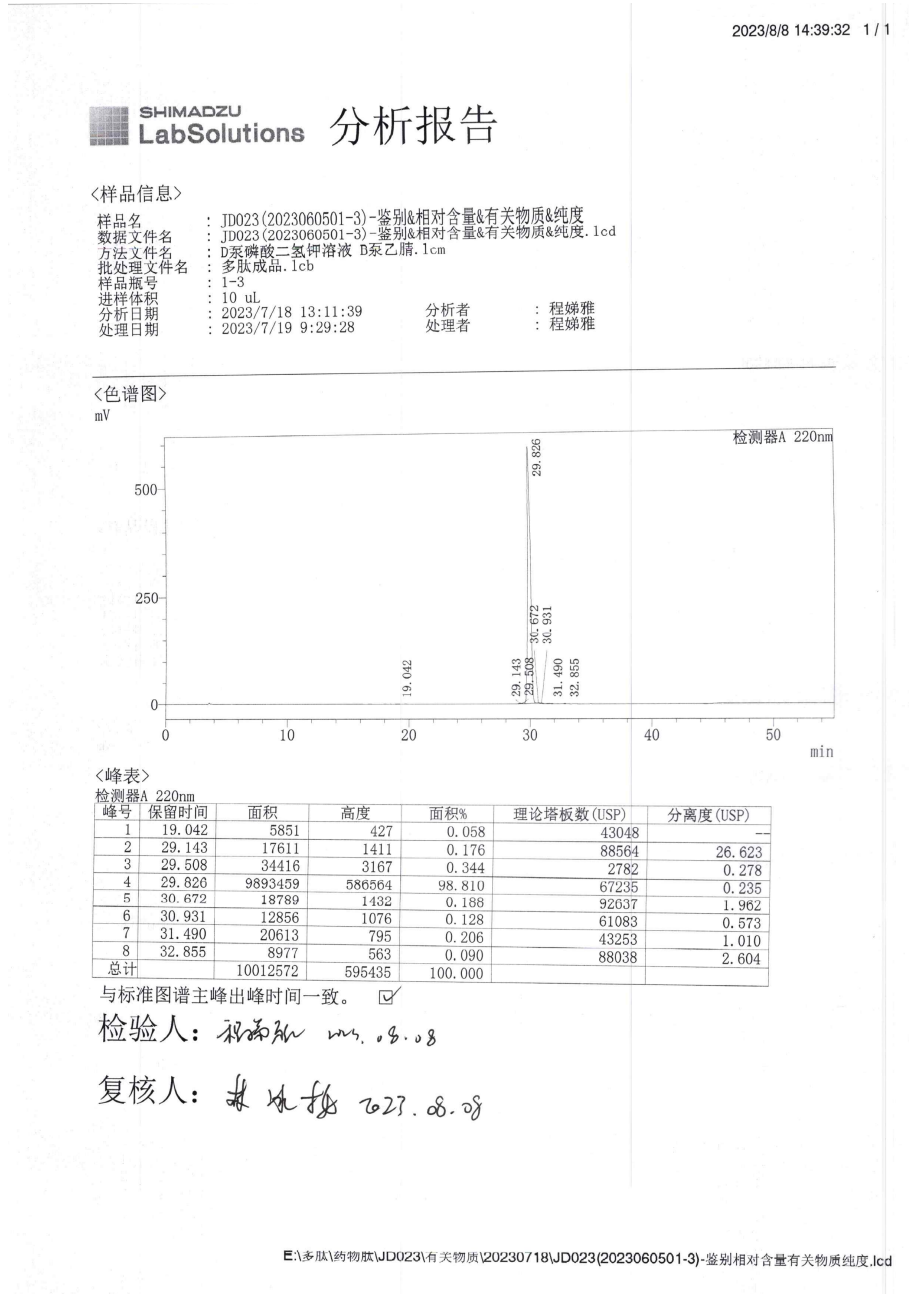

API Conforms to minimum purity requirements (99.810%), api quantity adjustment of 0.1% is made for 100%+ target.

- Chris Kamaras

